

## **ULR-10 OEM Integration Manual**

### **Universal Laser Systems, Inc.**

16008 North 81st Street  
Scottsdale, AZ 85260  
Phone: 480-483-1214  
Fax: 480-483-5620

**April 2010**

## Notice

This publication and its contents are proprietary to Universal Laser Systems, Inc. (ULS), and are intended solely for the contractual use of ULS, Inc. customers.

While reasonable efforts have been made to assure the accuracy of this manual, ULS shall not be liable for errors contained herein or for incidental or consequential damage in connection with the furnishing, performance, or use of this material.

ULS reserves the right to revise this manual and make changes from time to time without obligation by ULS to notify any person of such revision or changes.

ULS does not assume any liability arising out of the application or use of any products, circuits, or software described herein. Neither does it convey a license under its patent rights nor the patent rights of others.

This publication and its contents may not be reproduced, copied, transmitted, or distributed in any form, or by any means, radio, electronic, mechanical, photocopying, scanning, facsimile, or otherwise, or for any other purpose, without the prior written permission of ULS.

Intended use of this product must be followed within the guidelines of this manual. In no event will ULS be liable for any damages caused, in whole or in part, by customer, or for any economic loss, physical injury, lost revenue, lost profits, lost savings or other indirect, incidental, special, or consequential damages incurred by any person, even if ULS has been advised of the possibility of such damages or claims.

**WARNING: Universal Laser Systems products are not designed, tested, intended or authorized for use in any medical applications, surgical applications, medical device manufacturing, or any similar procedure or process requiring approval, testing, or certification by the United States Food and Drug Administration or other similar governmental entities.**

The product described herein is covered under one or more of U.S. Patents: 5,661,746; 5,754,575; 5,867,517; 5,881,087; 5,894,493; 5,901,167; 5,982,803; 6,181,719.

**© 2004 Universal Laser Systems Inc.  
All Rights Reserved**

## Contents

Notice.....	1
Contents .....	2
1.0 Introduction.....	3
2.0 Specifications.....	4
3.0 Safety Issues .....	7
3.1 Laser Safety .....	7
3.2 Electrical Safety .....	7
3.3 Electromagnetic Interference .....	7
3.4 Contacts for Safety Information.....	8
4.0 A Brief Description of the Laser.....	9
5.0 UL OEM Laser Installation and Operation.....	10
5.1 Mounting Method .....	10
5.2 Electrical Connections .....	11
5.3 Power Requirements .....	14
5.4 Interlock Circuit .....	14
5.5 Laser Modulation .....	14
5.6 Laser Tickle .....	15
5.7 CLASS-IV Operation.....	16
6.0 Air Cooling .....	16
6.1 Ambient Temperature .....	18
7.0 Water Cooling.....	19
7.1 Water Connections.....	19
7.2 Coolant.....	20
7.3 Environmental.....	20
7.4 Chiller Capacity .....	20
7.5 Draining the Laser.....	20
8.0 Laser Beam Output .....	21

## **1.0 Introduction**

Thank you for choosing a Universal Laser Systems CO<sub>2</sub> laser for your application. ULS is committed to providing the marketplace with low cost CO<sub>2</sub> lasers, which take advantage of our patented technology to provide compact size, ease of integration and high performance. This integration manual will guide you through the process of installing a ULS laser into your equipment and provide you with the information you need to operate the laser. Please read this entire manual and familiarize yourself with its contents. If you need help, please feel free to call Universal Laser Systems and we will be happy to provide you with assistance.

## 2.0 Specifications

Specifications for the UL-10 OEM lasers are summarized below.

Parameter*	Model		
	ULR-10 (basic)	ULR-10 (air-cooled)	ULR-10 (water-cooled)
Rated Power**	10 W		
Wavelength	10.6 $\mu$		
Power Stability	$\pm 10\%$ after 15 minutes of CW operation		
M <sup>2</sup>	1.4 $\pm$ 0.2		
Beam Size (Near Field****)	4 $\pm$ 1 mm		
Beam Divergence (Full Angle)	5 $\pm$ 1 mR		
Polarization	Linear (Perpendicular to the laser base plate)		
Pointing Stability	200 $\mu$ R		
Optical Pulse Rise or Fall Time	120 $\pm$ 40 $\mu$ S		
Optical Delay Time	38 $\pm$ 10 $\mu$ S		
Optical Modulation	100% up to 5 KHz		
Modulation Signal Type	TTL Compatible		
Cooling	<b>Air (integrator must provide fans and shroud)</b>	<b>Air Cooling (built-in fan and shroud)</b>	<b>Water Cooling</b>
Weight	7.25 Lb. [3.3 kg]	8.6 Lb. [3.9 kg]	8.6 Lb. [3.9 kg]
<b>Environmental</b>			
Ambient Temperature***	50-95°F [10-35°C]		
Relative Humidity	< 90% (non-condensing)		
<b>Power Requirements</b>			
DC Input Voltage	48.0 VDC		
RMS Current (CW, including fan)	4 A		
Inrush Current	10 A, 300 $\mu$ S		

\* The above specifications are subject to change without notice.

\*\* Output power is guaranteed to exceed this level for a period of 24 months from the date of purchase, regardless of use..

\*\*\* At temperatures below 50°F [10°C] operation may be intermittent and there is a potential for damage to the power supply and optics.

\*\*\*\* Near Field is approximately 150mm from output-coupler.

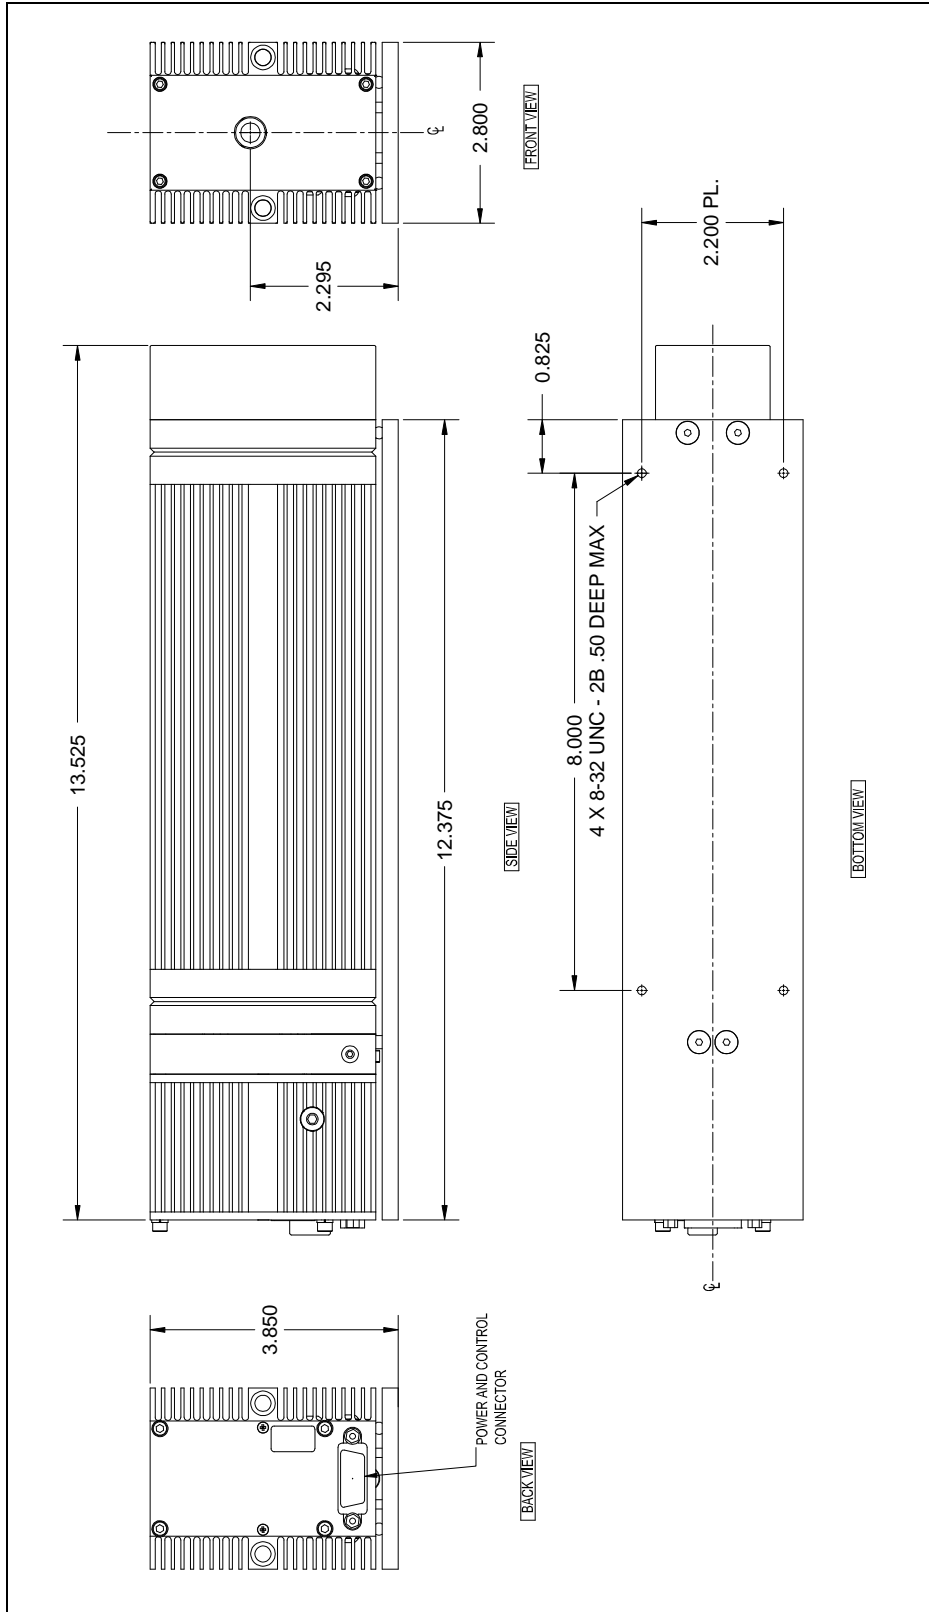


Figure 1 – Dimensional Specifications for Basic OEM Configuration

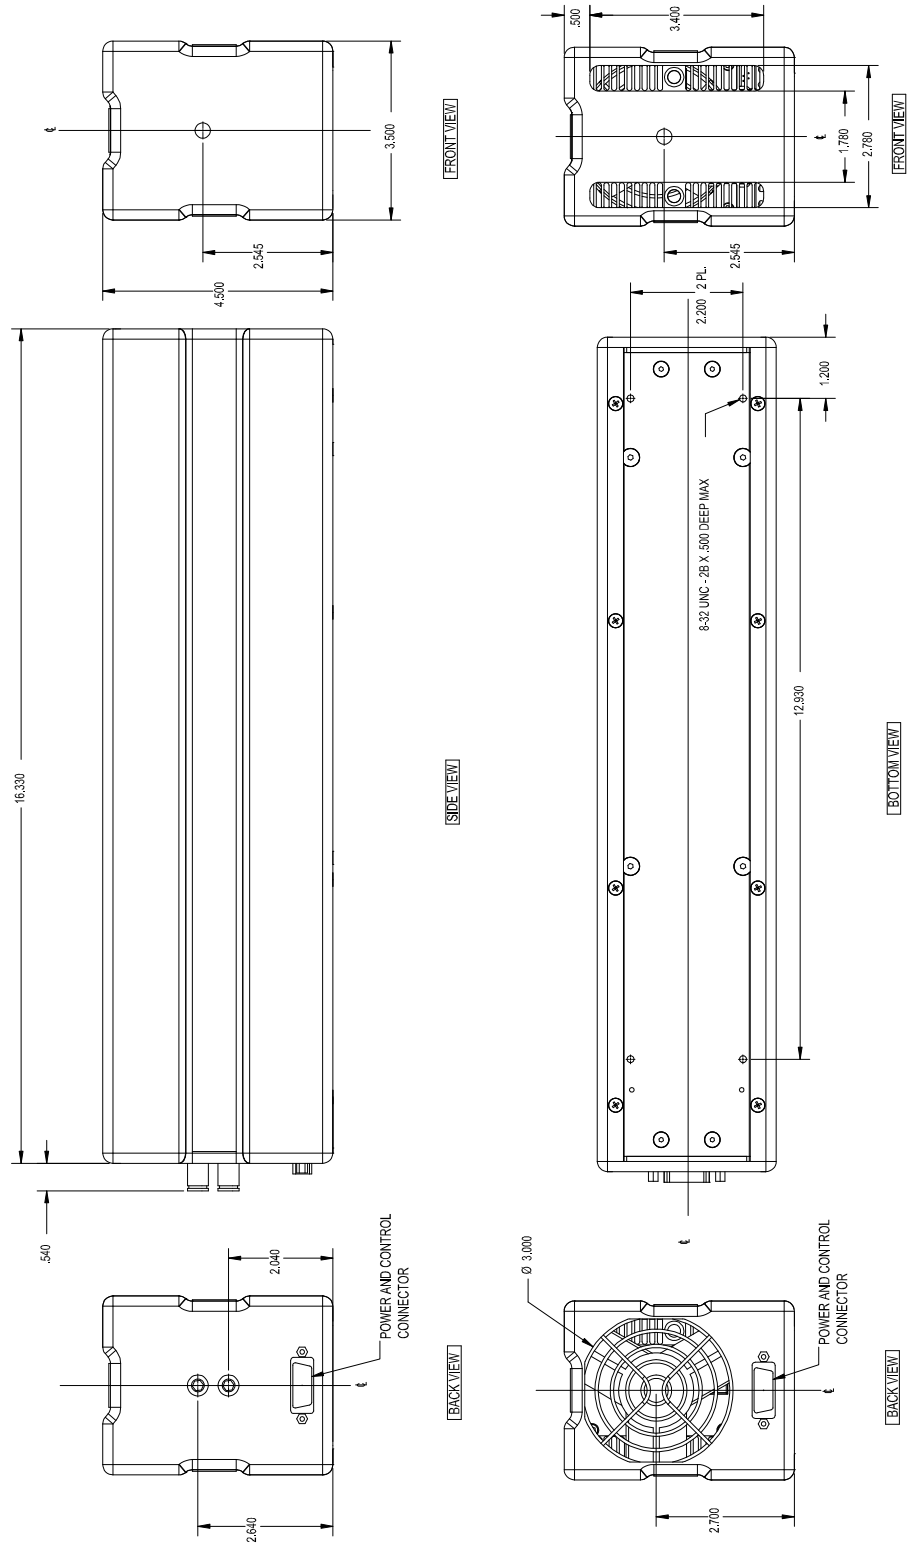


Figure 2 – Dimensional Specifications for Water and Air-Cooled OEM Configurations

## 3.0 Safety Issues

### 3.1 Laser Safety

ULS OEM lasers are sold as components and therefore are not required to conform to U.S. or European safety regulations. It is the responsibility of the buyer to design and certify any equipment incorporating a ULS OEM laser to meet all local safety regulations prior to sale to the public. The texts of these regulations are available from the respective governing bodies of the countries the equipment is to be sold into.

Any personnel working with or around open lasers must be aware of the following:

- **Exposure to the laser beam may cause physical burns and can cause severe eye damage.** Proper eye protection should be used at all times. All eye protection should be appropriate for the radiation wavelength generated by the laser in use.
- **Exposure to the laser beam may cause ignition of volatile or combustible materials.** Do not use lasers in the presence of these types of materials.
- **Never look directly into the laser output port.**
- **Interlock all rooms in which open beams may be present and post appropriate warnings on or near the doors.** Access to these rooms should be limited to properly trained technicians when lasers are in use.
- **Use appropriate protective coverings over all beam paths whenever possible.**
- **Lasers and optical elements should be positioned to keep the beam and reflections below eye level.**

*Notice:* For more information on EMI standards, refer to local EMI safety regulations.

### 3.2 Electrical Safety

ULS lasers operate at 48 VDC, which is below the voltage limit that is considered dangerous by most safety standards. However, the lasers draw large amounts of current and the power supplies needed to provide the 48 VDC usually require 90-240 VAC to operate. For these reasons, proper safety precautions should be taken with every portion of the electrical system.

*Notice:* For more information on EMI standards, refer to local EMI safety regulations.

### 3.3 Electromagnetic Interference

ULS OEM lasers are sold as components and therefore are not required to conform to all U.S. or European safety regulations regarding EMI. It is the responsibility of the customer to design and certify any equipment incorporating a ULS OEM laser to meet all local safety



regulations prior to sale to the public. However, testing by ULS has demonstrated that with a properly selected power supply and line filtering, all ULS OEM lasers will pass the relevant U.S. and European EMI standards for Class A equipment. See Section 5.3 for more information.

*Notice:* For more information on EMI standards, refer to local EMI safety regulations.

### **3.4 Contacts for Safety Information**

Below is a list of useful contacts for information on safety regulations in the U.S. Canada, and Europe:

#### United States

Food and Drug Administration - Center for Devices and Radiological Health (CDRH), 1-800-638-2041.

Federal Communications Commission (FCC), (301)362-3000.

Underwriters Laboratories Inc. (UL), Illinois (708)272-8800, New York (516)271-6200, California (408)985-2400.

Laser Safety Institute of America, (407)380-1553.

Occupational Safety and Health Administration (OSHA), (202)693-2300.

#### Canada

Canadian Standards Association (CSA), (416) 747-4000.

#### Europe

European Committee for Electrotechnical Standardization (Cenelec), rue de Stassart 35, B-1050 Brussels

International Organization for Standardization (ISO), 1 rue de Varembé, Case postale 56, CH-1211 Genève 20 Switzerland

## 4.0 A Brief Description of the Laser

This ULS OEM CO<sub>2</sub> gas laser uses a sealed-off, RF-excited, slab design and a multi-pass, free space resonator<sup>1</sup>. Each laser consists of a plasma tube, with mirrors at each end forming an optical resonator, and an RF power supply assembled together in a chassis with convenient mounting provisions. Various cooling arrangements using water or air are available.

The plasma tube consists of two opposing electrodes in a slab configuration, meaning the cross-section of the gap between the electrodes is rectangular instead of square. This allows for a multi-pass resonator in which the laser beam makes several passes within the plasma using the full width of the rectangular electrode gap. The advantage of this is a powerful laser beam from a relatively short tube.

The length of the gap between the electrodes is designed to allow free space operation of the laser. This means that the gap is wide enough to allow the laser beam to form without any substantial waveguide effects caused by reflection of light from the surfaces of the electrodes. This provides for a very good quality beam in the near field as well as far field.

The optical resonator is formed by a system of three mirrors, one in the back and two in the front, with one front mirror being partially reflective to allow the beam to exit the tube. These mirrors are tuned to specific angles to generate multiple passes of the laser beam within the plasma formed between the electrodes.

One of the electrodes is attached to the RF power supply through a matching network that allows the impedance of the tube to be tuned to match the impedance of the supply. The RF power supply operates at approximately 40 MHz. Power control of the laser beam is provided through pulse width modulation of the RF by an external TTL signal provided by the user.

---

<sup>1</sup> As described in U.S. Patent 5,661,746

## 5.0 UL OEM Laser Installation and Operation

### 5.1 Mounting Method

Each version of the ULR-10 OEM laser contains 4 threaded holes in its base plate for mounting the laser. The dimensions for these hole patterns is given below. It is recommended that the screws not extend more than 0.50" [12.7 mm] into the laser. The laser can be mounted in any orientation including vertical. Dimensions for the mounting-hole pattern are given below. The laser should be mounted using a three-point arrangement to avoid warping or bowing the assembly. If the laser is mounted on a flat surface it should be flat to within 0.025 inches [0.65 mm].

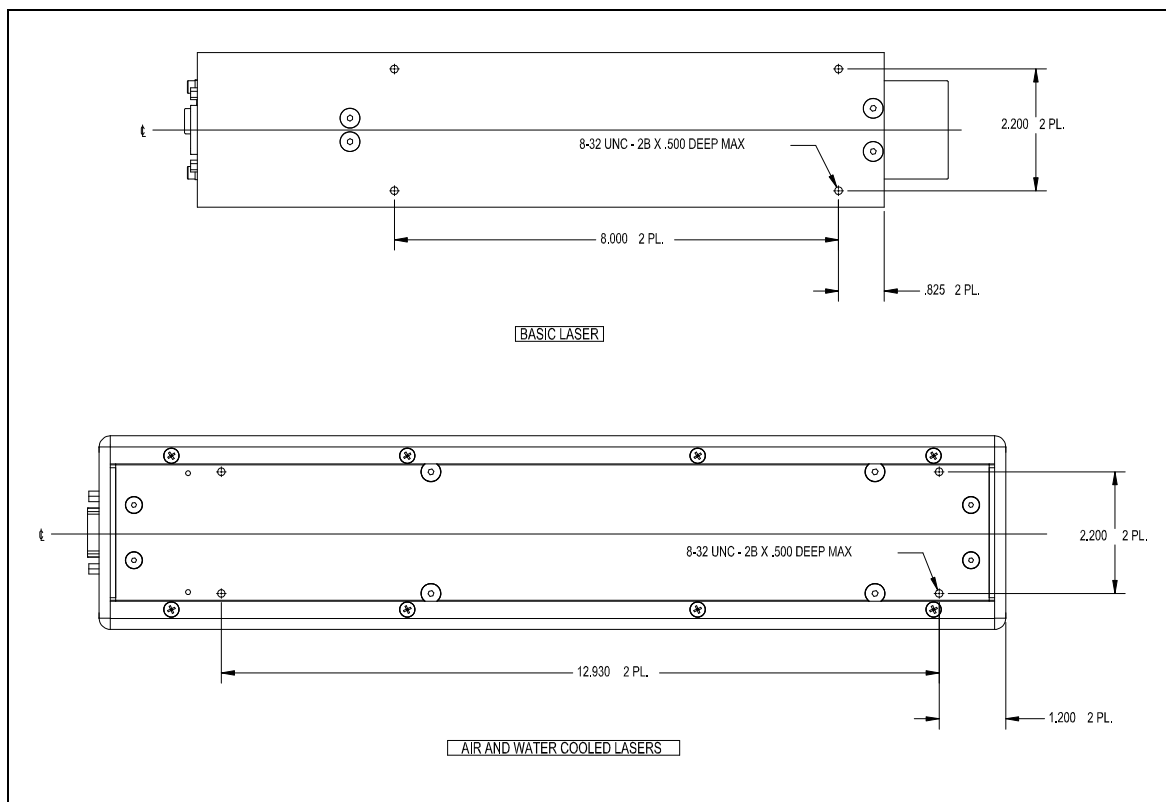


Figure 3 - Detail of Mounting Hole Dimensions

## 5.2 Electrical Connections

All electrical and communication connections for the laser are made through one fifteen-pin connector located on the back of the laser. Figure 4 below shows the pin positions of the mating connector on the wire harness. Figure 5 details the circuits inside the laser attached to the pins.

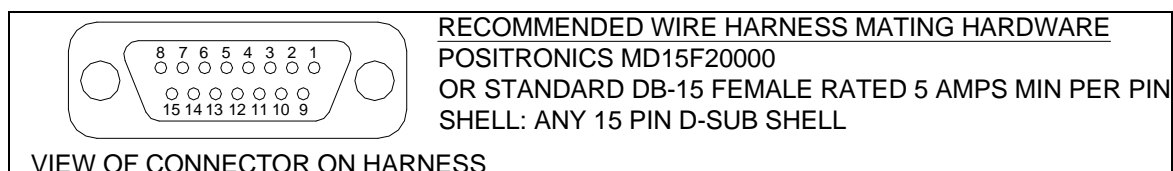



Figure 4 – Laser Connector Pin Diagram

Pin Number	Input Name	Laser Input/Output	Wire Size	Description
1	+48V	Power input	20 AWG	+48 volt power; do not swap polarity. <sup>1</sup>
2	Laser Diode	Optically isolated input	20-24 AWG	+5 V signal on pin 2 will turn on the red laser pointer (when available).
3	Temperature Warning <sup>5</sup>	TTL Output	22 AWG [0.33mm <sup>2</sup> ]	HI= Normal Low= Fault Return on pin 14
4	Modulation +	Optically isolated input	20-24 AWG	Laser modulation signal is connected between pins 4 and 12.
5	Laser Diode Return	Optically isolated input	20-24 AWG	Optically isolated return signal for “Laser Diode” (pin 2). <sup>3</sup>
6	Interlock +	12 volt source (only use for interlock)	20-24 AWG	Connect safety switches between pins 6 and 13 to enable laser. Do not use this pin as a power source for other purposes.
7	Laser Status	TTL Output	20-24 AWG	TTL Output. Return on Pin 14
8	Power Ground	Power input	20 AWG	Power ground. <sup>2</sup>
9	+48V	Power input	20 AWG	+48 volt power; do not swap polarity. <sup>1</sup>

10	+D	RS485 +	20-24 AWG	Half-duplex communication port.
11	-D	RS485 -	20-24 AWG	Half-duplex communication port.
12	Modulation -	Optically isolated return signal	20-24 AWG	Optically isolated return signal for "modulation +" (pin 4). <sup>3</sup>
13	Interlock -	Interlock return	20-24 AWG	See description for Pin 6.
14	Signal Return	Ground reference	20-24 AWG	Return for "Laser Status +" (Pin 7), Temp warning Pin 3 RS485 ground reference and externally sourced interlock.
15	Power Ground	Power input	20 AWG	Power ground. <sup>2</sup>

## Notes:

1. Pins 1 & 9 are internally connected, and it is recommended that both pins be connected to the external power supply.
2. Pins 8 & 15 are internally connected, and it is recommended that both pins be connected to the external power supply return.
3. Pins 5 & 12 are internally connected. This ground is capacitively coupled to chassis ground and is provided as an isolated ground for the customer.
4. Pins 7 & 14 are TTL and can source up to 20mA.
5. Temperature warning operates in the following manner:
  - Temperature exceeds 60C: Pin 3 goes low as a warning. The laser will continue operating.
  - Temperature exceeds 70C: Pin 7 goes low as a fault. The laser will stop operating.
  - After over-temp:
    - a. Temperature falls below 60\*C: Pin 3 goes high. Laser still does not operate.
    - b. Temperature falls below 48\*C: Pin 7 goes high. Laser able to operate if modulation is applied.
  - On initial power-up:
    - a. Temperature is below 0\*C: Pin 7 goes low as a fault. Laser will not operate.
    - b. When temperature is above 0\*C: Pin 7 goes high. Laser able to operate if modulation is applied.
  - 0\*C is not monitored if laser is already running as the gas is energized and low temperature shouldn't cause problems.

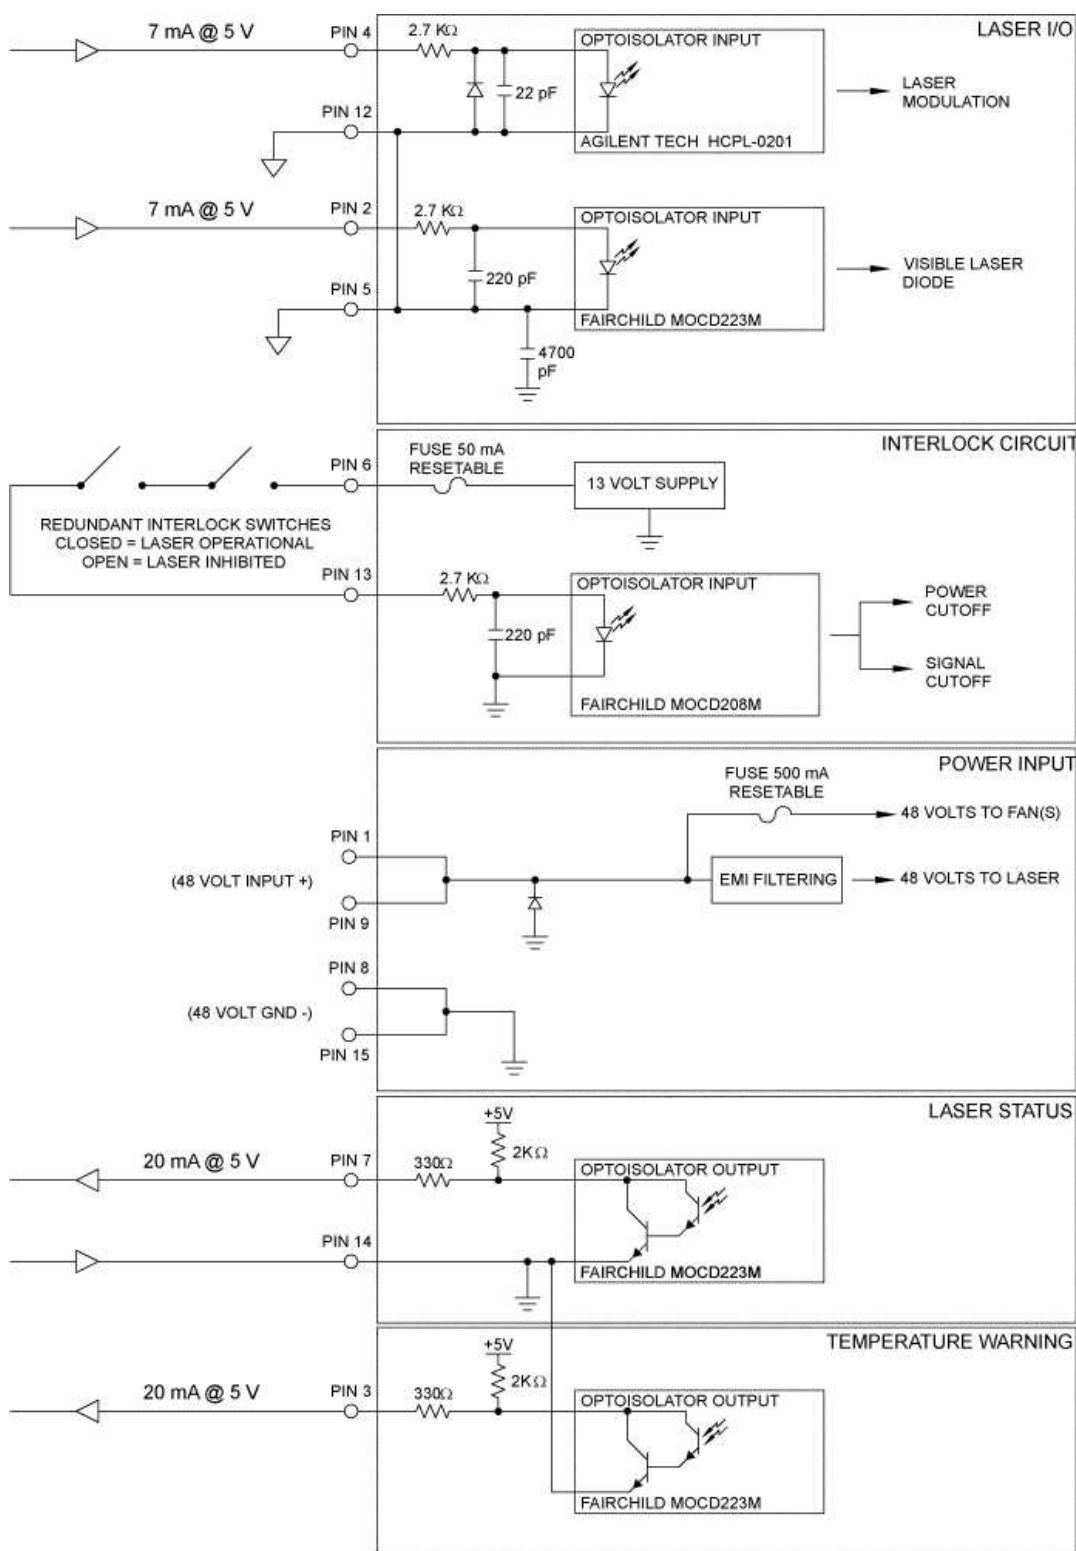

NOTE - ALL CIRCUITS OUTSIDE THE DASHED LINES ARE EXAMPLES TO ILLUSTRATE THE PROPER METHODS FOR INTERFACING WITH THE LASER.

Figure 5 – Laser Interconnect Schematic

### 5.3 Power Requirements

A good quality 48 volt DC power supply should be used to power the laser. Nominal output should not exceed 48 volts and regulation should be within 0.5% under 100% load. The power supply should have good transient response characteristics to handle the fluctuating current requirements caused by modulation of the laser. The power and signal connector provides 48 volts and ground connections to the power supply. One 20 AWG [.82 mm<sup>2</sup>] wire should be used on each of the power and ground pins (pins 1,8,9,15). Careful attention should be paid to power entry filtering when designing to meet Class A conducted EMI regulations. In order to meet Class A emitted EMI regulations, it is important that the 48 volt power wires be no more than 3 feet (1 meter) in length and that the 48 volt power supply and laser chassis be attached to a common earth ground through very low induction connections. Finally, it is advisable to use shielded wiring for all I/O connections to the laser.

### 5.4 Interlock Circuit

An interlock circuit is incorporated into the laser, which can be combined with external switches to satisfy safety requirements when designing Class 1 laser equipment. At least two redundant switches must be used for each panel providing access to a Class 1 enclosure. Please refer to the appropriate safety regulations for more information on Class 1 laser equipment design.

The interlock circuit is self-sourced using a 12 volt output supplied by the laser on pin 6. The interlock is shunted by connecting pin 6 to pin 13 allowing the laser to operate. Any break in this connection will cause the laser to stop operating. Switches can be placed in series with these pins to create a safety interlock circuit.

### 5.5 Laser Modulation

A TTL compatible signal must be provided to pin 4 to drive the laser. Output power can be controlled from 0 to 100% (CW Mode) by pulse width modulation of the input signal. The electrical requirements for the modulation signal are as follows:

Nominal Voltage	5 Volt (7 volts max)
Current	7 mA Min
Logic high	2.70 Volts Min
Logic Low	1.725 volts Max

As with all CO<sub>2</sub> lasers, delays are inherent in the response of the laser beam output to the input signal. A typical laser will have response characteristics similar to those detailed in the oscilloscope traces in figures 6 and 7 below. These figures show a TTL signal and corresponding laser power output.

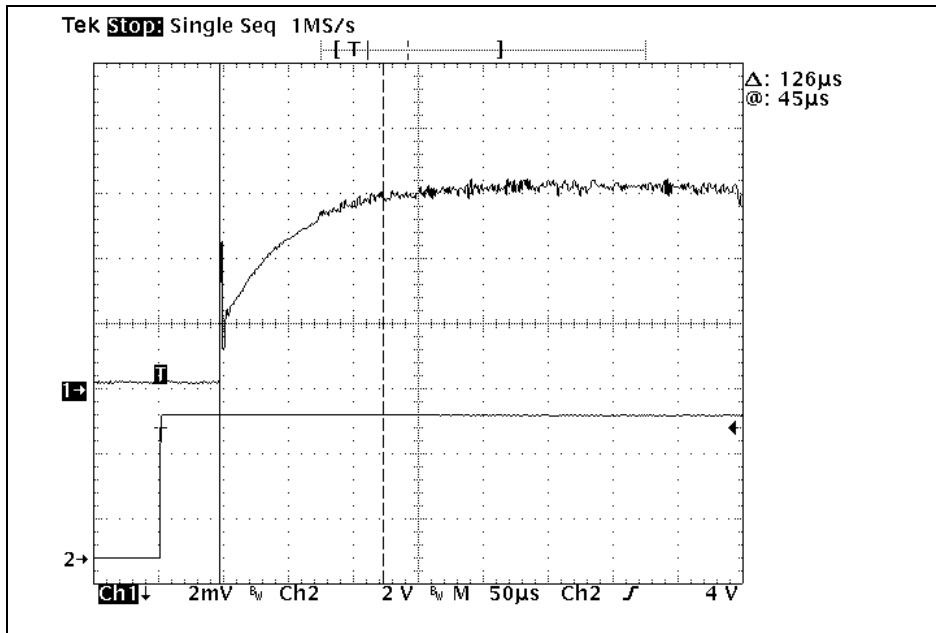


Figure 6 – Oscilloscope trace of typical rise time for a laser

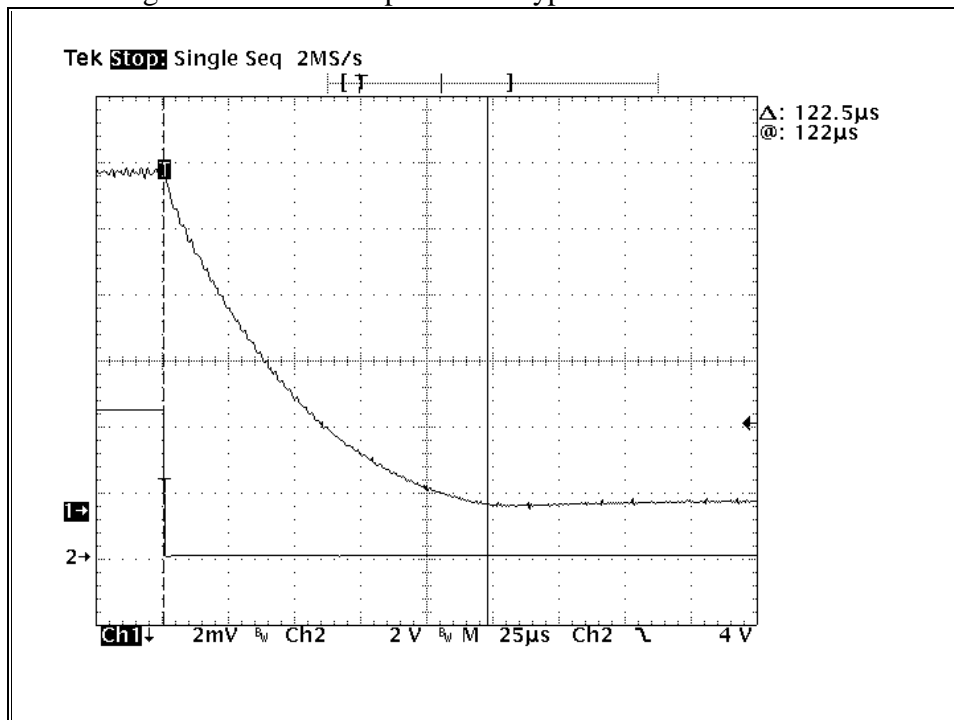


Figure 7 – Oscilloscope trace of typical fall time for a laser

## 5.6 Laser Tickle

It is a common practice with CO<sub>2</sub> lasers to provide some means of stimulating the mixture when the laser is off in order to improve its response. ULS lasers have a built-in, low duty cycle, secondary modulation signal called a tickle signal to accomplish this effect. This



signal is pre-tuned at the factory for optimal performance of the laser and normally does not require adjustment.

### **5.7 CLASS-IV Operation**

Lasers configured for CLASS-IV operation are equipped with a key-switch and interlocked shutter. The shutter is manually actuated with a lever located on top of the laser near the beam-exit end. When closed, a solid metal shield blocks the beam exit of the laser, and a mechanical interlock switch is opened which will prevent the laser from emitting. The shutter is marked with OPEN and CLOSED so the user can see its present status without being exposed to laser radiation. An emission LED indicator is located on the opposite end of the laser from the beam output. When illuminated, emission is possible if a signal is applied to the modulation pin. A key-switch with removable key is located on the opposite end of the laser from the beam output. In the off position, this switch will open the laser interlock circuit, preventing the laser from emitting. When the key-switch is closed, there is a 4 second delay before the laser is capable of emitting. In Class-IV configuration, any time the interlock circuit is opened, the key switch must be turned to the “off” position and back to the “on” position before the laser is capable of emitting (provided the interlock is closed). The 4-second emission delay applies in this case as well.

### **6.0 Air Cooling**

Careful attention should be paid to proper airflow through the laser (see figures 8 and 9) when integrating it into equipment. The ULR-10 OEM laser is available in two air-cooled versions: The basic version in which the fans and air flow shroud are not supplied and the air-cooled version in which the fan and shroud are included. With either version, any restriction of airflow will result in reduced power output and can cause permanent power loss or failure over extended periods of time. Ambient air should be directed to the laser’s air flow intake, and exhaust air from the laser should be directed out of equipment with as little restriction as possible. If the laser is placed in an enclosure, it may be necessary to provide additional fans to draw exhaust air out of the enclosure to reduce a rise in temperature inside the enclosure, which can affect laser output power. The exhaust air should be no more than about 10°C above ambient.

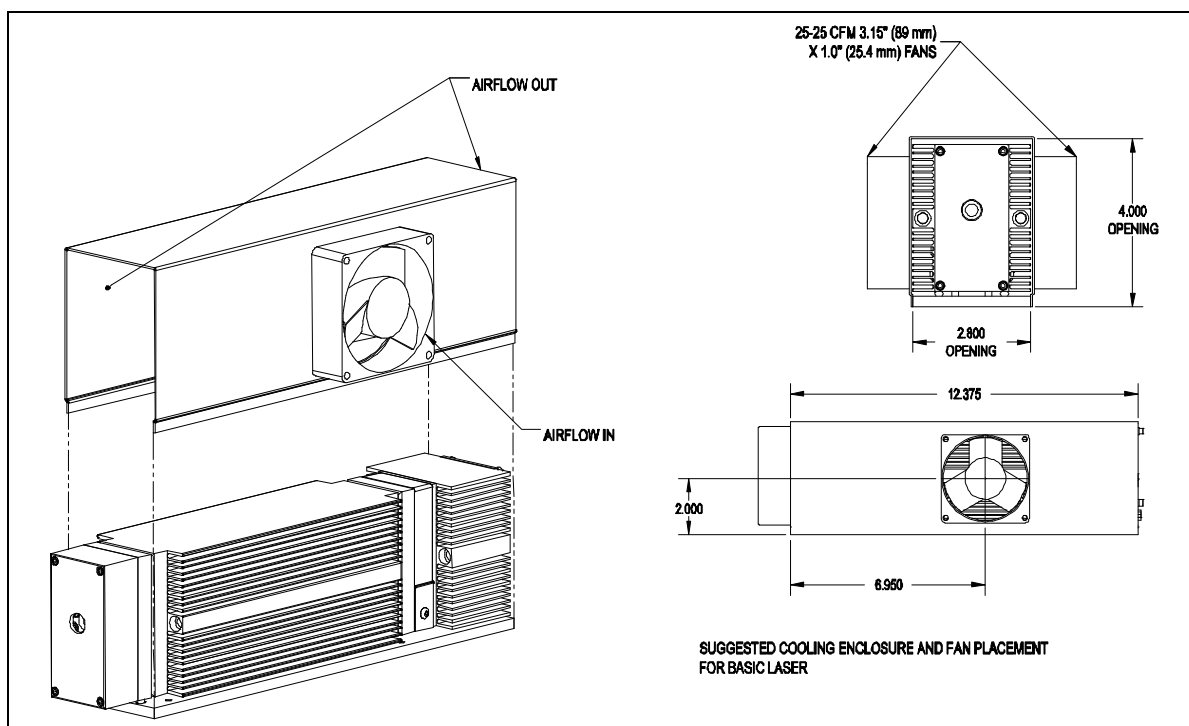


Figure 8 – Detail of Air Flow Through the Basic Laser

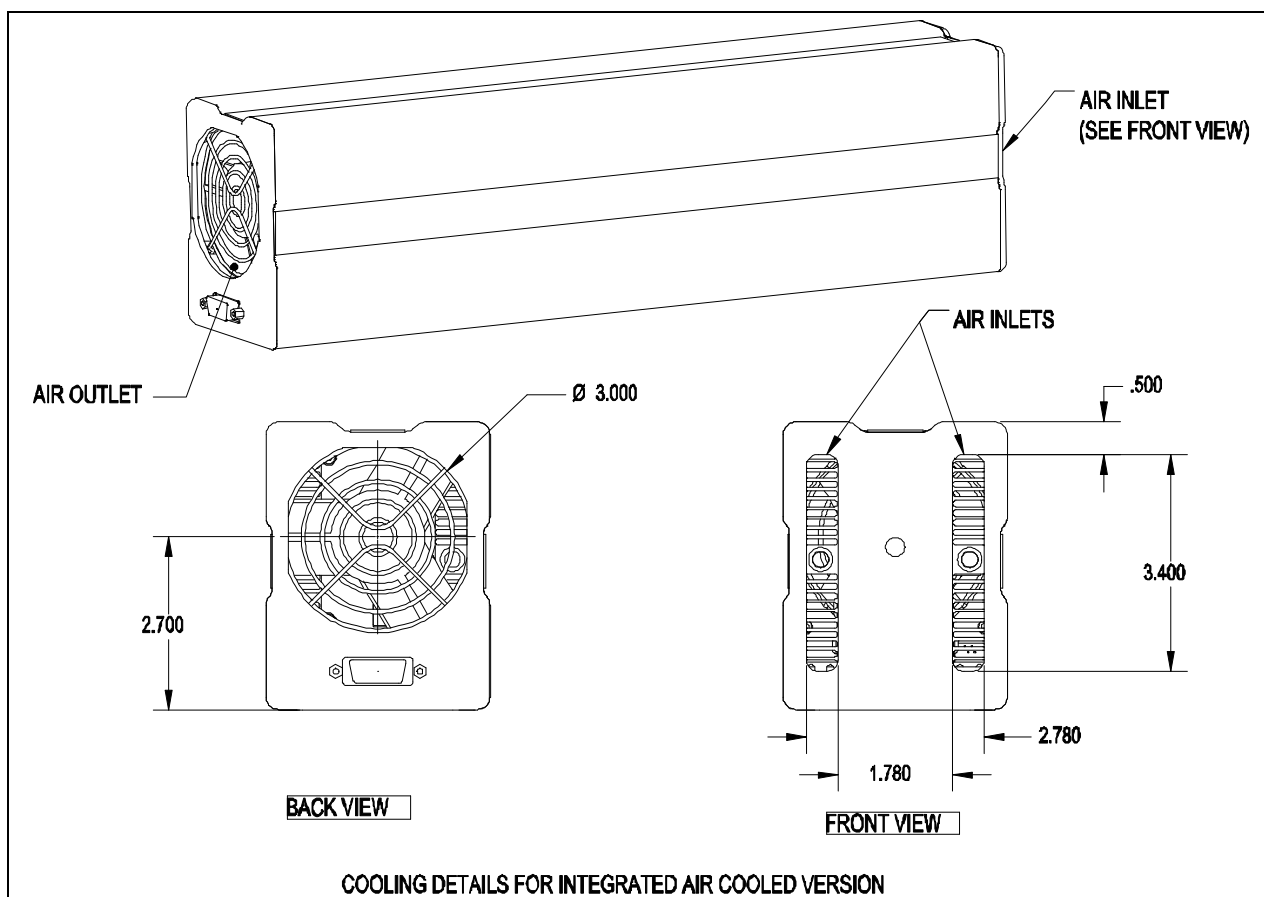


Figure 9 – Detail of Air Flow Through the Air Cooled Laser

Finally, ambient air should be filtered before entering the laser to prevent a buildup of dust and debris on the cooling fins which can reduce cooling efficiency, however, care should be taken when selecting a filter media to ensure that the filter does not restrict air flow. For relatively clean environments, a low restriction filter media (45 pores per inch, for example) might be adequate, but for dirtier environments a heavier filter media might be required and also a booster fan can be employed on the exhaust end to help pull air through the laser.

### 6.1 Ambient Temperature

Air-cooled lasers by nature are sensitive to ambient temperatures. Hotter ambient temperatures will reduce power output and cooler ambient temperatures will increase power output. An ambient temperature range of 50-95°F [10-35°C] should be observed to guarantee proper laser operation. At temperatures below 50°F [10°C] operation may be intermittent and there is a potential for damage to the power supply and optics. At temperatures above 95°F [35°C] ULS lasers are not guaranteed to provide the rated power output. Lasers can safely be operated at ambient temperatures above 95 °F [35°C], however, power output will diminish as ambient temperature rises and longevity can be significantly reduced.

## 7.0 Water Cooling

### 7.1 Water Connections

ULS 10-Watt water cooled lasers are equipped with two “Instant Tube Fittings” for 1/4” OD tubing. Attempting to connect metric tubing directly to these fittings will result in leakage. To connect tubing to this fitting, make sure the tubing is squarely cut and push the tubing into the fitting until it stops (.7” - .8” insertion), then pull the tubing to ensure it is locked. Connect the OUT on the coolant source to the IN on the laser and the OUT on the laser to the IN on the coolant source (Please refer to Figure 10).

To remove the tubing from the fitting, push the orange plastic ring towards the fitting. Hold the ring in while pulling the tubing out. To ensure a good connection, we recommend that after removing tubing from a fitting, the tubing be trimmed 1” from the end so that un-inserted length of tubing is re-inserted into the fitting.

Take care to not kink the tubing as this will restrict coolant flow and can weaken the tubing.

*Note: ULS water cooled lasers may be shipped with plugs in the water fittings. Remove these prior to installation of tubing.*

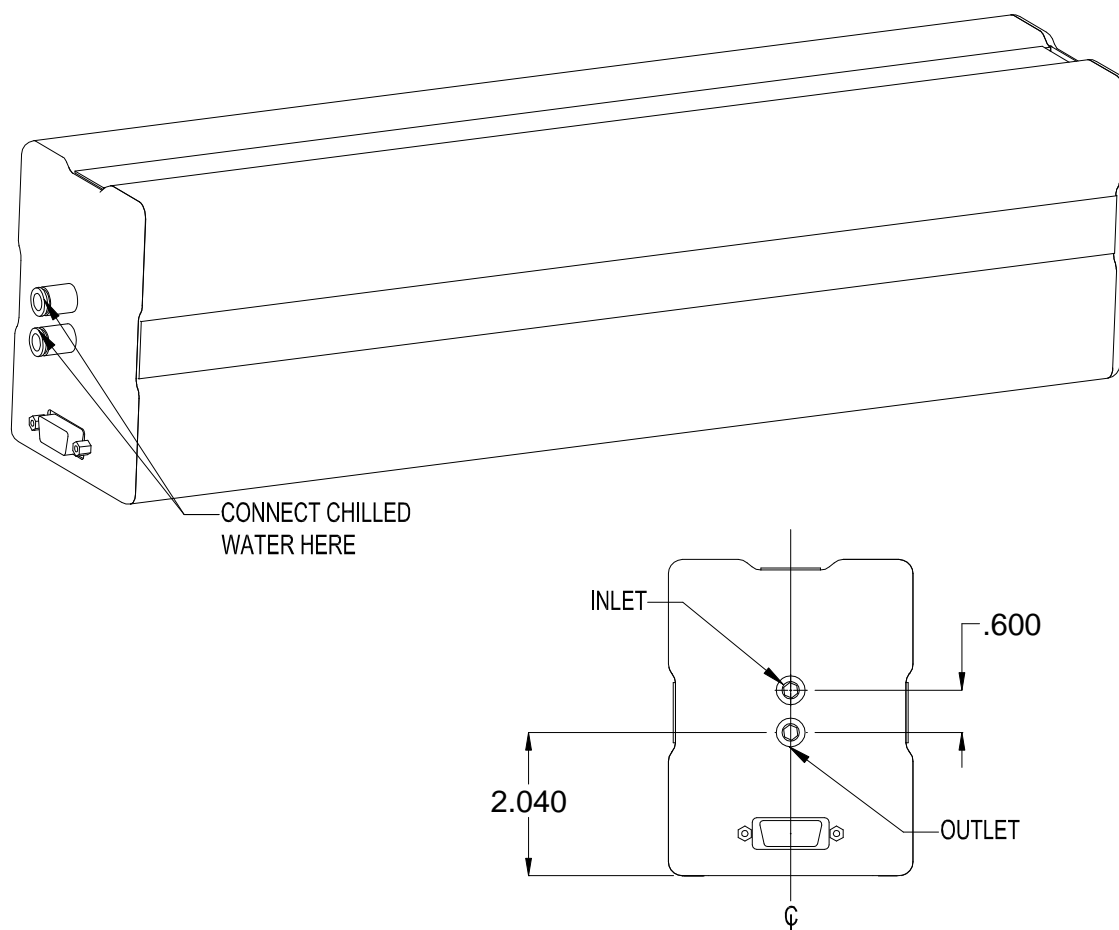


Figure 10 – Detail of Water Cooled Laser

## 7.2 Coolant

ULS lasers are designed to be used with distilled water. Do not use de-ionized water. Glycol-based coolants or additives are not necessary for use in ULS water cooled lasers as the lasers should not be operated below 50°F [10°C]. If the laser is connected to a closed-loop system, ULS recommends adding an algacide/anti-corrosive such as Optishield Plus to the coolant. Do not exceed a coolant pressure of 60psi.

## 7.3 Environmental

The environment that ULS Water Cooled lasers operate in can affect their longevity and operation. Condensation forming on the laser can cause damage to optics and electronics, degrading performance or causing laser failure. Therefore it is important to set the coolant temperature properly.

The temperature at which airborne water vapor will condense on a surface is the dew-point. The dew-point is determined by air temperature and relative humidity. If the laser is cooled at or below the dew-point, condensation will form on the laser. The table below shows dew-point values for various temperature and relative-humidity values.

		Relative Humidity								
		10%	20%	30%	40%	50%	60%	70%	80%	90%
AIR TEMP	10°C	-20.2	-11.9	-6.8	-3.0	0.1	2.6	4.8	6.7	8.4
	15°C	-16.4	-7.8	-2.4	1.5	4.7	7.3	9.6	11.6	13.4
	20°C	-12.5	-3.6	1.9	6.0	9.3	12.0	14.4	16.4	18.3
	25°C	-8.7	0.5	6.2	10.4	13.8	16.7	19.1	21.3	23.2
	30°C	-4.9	4.6	10.5	14.9	18.4	21.4	23.9	26.2	28.2
	35°C	-1.2	8.7	14.8	19.4	23.0	26.0	28.7	31.0	33.1

The orange values are the dew point temperatures (in °C). For example, at an ambient temperature of 25°C with 40% Relative Humidity, the dew-point temperature is 10.4°C. The coolant temperature should be kept above this dew-point temperature to avoid condensation on the laser.

## 7.4 Chiller Capacity

For the ULS Water Cooled 10W laser, we recommend a minimum chiller cooling capacity of 300 Watts. We recommend a minimum of 1 gallon per minute flow rate.

## 7.5 Draining the Laser

When shipping a Water Cooled ULS tube, you must ensure that the laser is free of coolant. During shipping, temperatures can reach below freezing. If coolant freezes inside the laser tube, catastrophic damage can occur. To drain the tube, first insert short pieces of tubing into each water fitting, placing the ends of the tubes in a suitable reservoir or drain. Place the laser on a clean, water-resistant surface, so that the water fittings are nearest to the surface it is resting on. Allow the tube to drain completely. After draining, insert the plugs that the laser was shipped with into the water fittings.

## 8.0 Laser Beam Output

The beam exits the laser as detailed in Figure 11. When integrating a laser with external optics or a beam delivery system, care should be taken to seal the beam path in order to prevent contamination of the laser's optics. Laser optics are exposed to the environment through the beam exit aperture on the laser. Failure to protect laser optics from dust, fumes and debris will cause premature failure of the laser and can void the warranty.

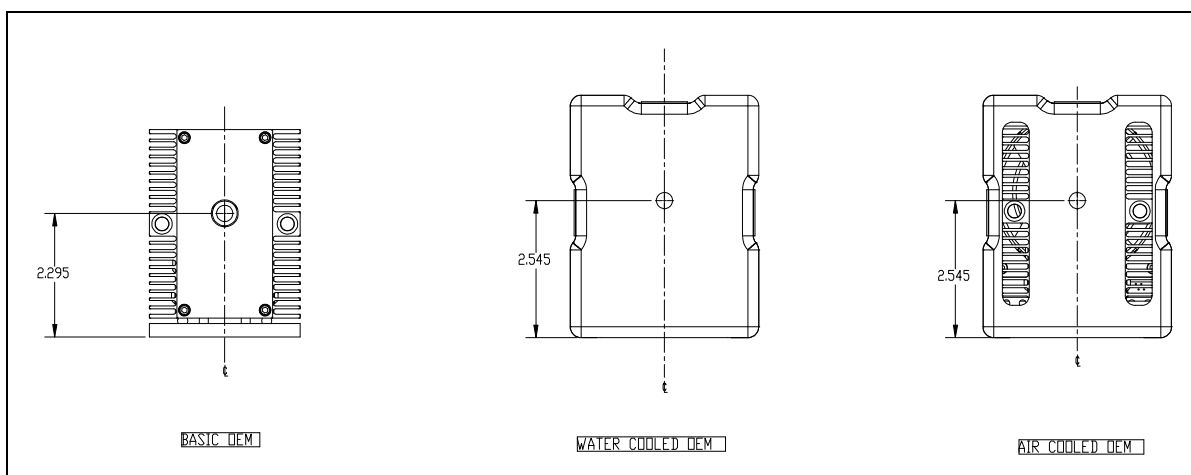


Figure 11 – Detail of Beam Output