

This document is intended to act as a guide to ensure that your facility is ready to accept your new laser system and to facilitate a seamless installation. This document provides a list of requirements that must be completed or verified before the installation of your laser system to avoid any delays during installation or additional charges.

This document must be fully completed, signed, and returned to sitesurvey@ulsinc.com to schedule an installation date. If you have any questions or concerns, please contact your ULS Representative or sitesurvey@ulsinc.com.

PART A – System Location Information

INSTALLATION LOCATION

Please provide details for the final system location. This is where the installation will take place.

COMPANY NAME

STREET ADDRESS

CITY

STATE

ZIP

COUNTRY

CONTACT NAME

TITLE

PHONE NUMBER


EMAIL ADDRESS

NOTES (IF APPLICABLE)

PART B - Operational Considerations & Requirements


FLOOR SPACE UTILIZATION

System dimensional drawings:

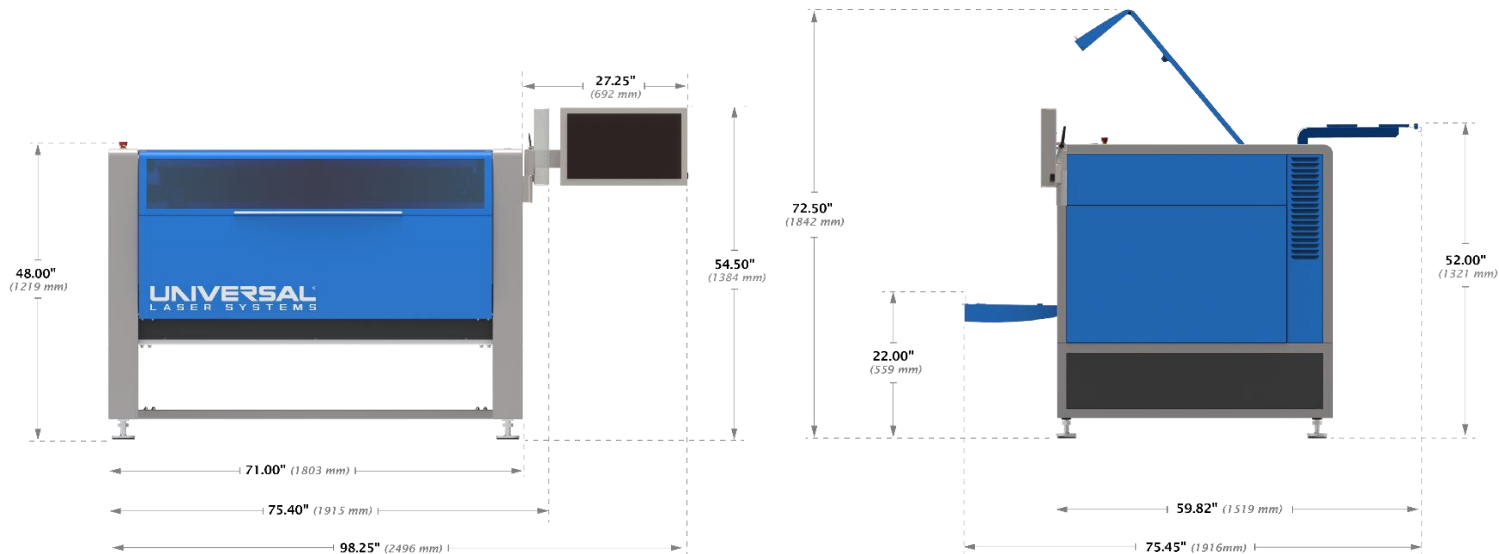


FRONT VIEW WITH AVAILABLE TOUCH SCREEN CONTROL PANEL

SIDE VIEW DOORS OPEN WITHOUT CONTROL PANEL

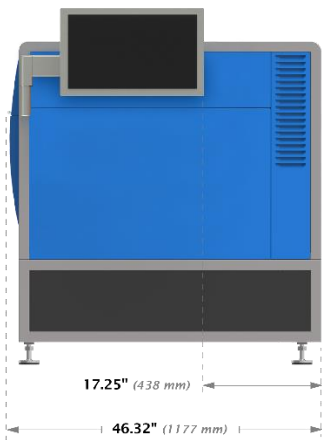


SIDE VIEW WITH AVAILABLE TOUCH SCREEN CONTROL PANEL FOLDED


Ensure the system is set in a location with a minimum clearance of 2' (610 mm) on each side and overhead as shown below:



Width 147"
(3734 mm)
(119" (3023 mm) without control panel)



Depth 123"
(3125 mm)



Height 97"
(2464 mm)

ENVIRONMENTAL REQUIREMENTS

The ULTRA R9000 system requires a well ventilated environment with a noncondensing humidity level between the temperatures of 50° F (10° C) to 95° F (35° C). An optimal temperature range of 73° F (22° C) to 77° F (25° C) is recommended for peak performance.

Does your facility meet the environmental requirements? ☐ YES ☐ NO*

**If NO, provide date requirements will be met:* _____

EXHAUST REQUIREMENTS

An exhaust blower or air filtration system is required.

If installing an UAC 4000 air filtration system, verify a separate 220 VAC power receptacle is available. The UAC 4000 is specifically designed for integration with ULTRA laser processing systems. If using a third-party filtration system, consult the manufacturer for recommendations.

If an exhaust blower will be used it must be capable of moving at minimum 700 cubic feet per minute (CFM) of air at 6 inches of static pressure (1190 m³/hour at 1.5 kPa) through a 6-inch (152.4 mm) duct or flexible hose where it connects to the ULTRA R9000 system. When planning an exhaust system, it is essential to consider the length of the duct/flexible hose from the exhaust blower to reach the laser system without tension while also accounting for pressure loss over a long distance. (The blower rating above is intended to allow for 250 - 300 cfm (425 – 510 m³/ hour) airflow at 1.5" (.15 kPa) static pressure through the ULTRA R9000.)

All exhaust solutions must meet local codes and regulations. Consult registered local contractors or exhaust experts if necessary.

Does your facility meet the exhaust requirements? ☐ YES ☐ NO*

**If NO, provide date requirements will be met:* _____

ADDITIONAL REQUIREMENTS (USER SUPPLIED)

- A regulator will be required if facility compressed air is utilized. The compressed air should be instrument quality, filtered clean, dry and oil-free. Air requirement is 100 psi max pressure and 3 CFM free airflow (3.4 bar and 5 cubic meters/hour). The connection is a quick-release fitting that accepts ¼ inch NPT connection.
- If a compressed gas (required non-flammable gas such as Nitrogen) is used, a regulator will be required to supply gas at 100 psi max (6.8 bar). Connection is a fitting that accepts ¼ inch NPT connection.

- Minimum computer requirements (if not configured with available 21" Touch Screen Control Panel) are as follows: Intel i3 processor (or equivalent) with at least 8 GB (16 GB recommended) of memory, Windows 10 or Mac 10.15 (Catalina) operating system, USB 3.0 or USB SuperSpeed (SS) port and USB cable for connection to the laser system.
- Avoid placing the laser system under direct lighting. Glare from lighting can adversely affect camera registration results.

Will the system be placed under direct lighting? ☐ YES* ☐ NO

Does your facility meet these additional requirements? ☐ YES ☐ NO*

**If NO, provide date requirements will be met:* _____

CLASS 4 SAFETY NOTICE

There are specific legal regulations that must be adhered to when operating in Class 4 mode. You must provide interlocked entrances and illuminated indicator signs outside the room. A trained Laser Safety Officer (LSO) must be designated, and the laser system registered with the appropriate agencies.

If the Class 4 Conversion Module for Pass-Through was purchased, you must read the Class 4 Acknowledgement in full. Sign and return the Class 4 Acknowledgement to ULS before receiving an installation date.

POWER REQUIREMENTS

The system location requires facility power receptacles for the items listed below.

A. ULTRA R9000

- **Standard Configuration** - 208/230 VAC, 16 A, 50/60 Hz single-phase dedicated circuit (a dedicated 20 or 30 A outlet recommended)
- **High Power Configuration (dual 150-watt laser sources)** - 208/230 VAC, 25 A, 50/60 Hz single-phase dedicated circuit (a dedicated 30 A outlet recommended)



SHOWN WITH AVAILABLE TOUCH SCREEN CONTROL PANEL

B. ULS Compressed Air Source* – 110 VAC at 10 A or 220 VAC at 5 A

Please select: ☐ 110 VAC ☐ 220 VAC



C. Vacuum Booster* – 110 VAC at 10 A or 220 VAC at 5 A; auto-switching

Please select: ☐ 110 VAC ☐ 220 VAC



**Available feature*

Note, you must supply appropriate plugs for all 220 VAC facility power receptacles (for example L6-30 plug). The service technician will connect the plug(s) to the equipment cable(s) during installation.

Does your facility meet the power requirements? ☐ YES ☐ NO*

**If NO, provide date requirements will be met: _____*

PART C - System Receiving and Transport Considerations

SYSTEM CRATE AND TRANSPORT

The ULTRA R9000 system will arrive in a crate with dimensions of 60" x 75" x 87" (1524 x 1905 x 2210 mm) and will weigh as much as 1,100 lbs. (499 kg). Please indicate in the following questionnaire if you have a receiving dock. Please indicate if a liftgate is required on the delivery truck.

A forklift with extensions is recommended to remove the ULTRA R9000 system from the crate and move it through your facilities. If a forklift is not available, it is strongly recommended a rigging company be available to remove and relocate the laser system. A pallet jack can also be used to move the laser system through your facility.

SYSTEM RECEIVING

1. Is a receiving dock present at the delivery site? ☐ YES ☐ NO

2. Will a rigging company be required? ☐ YES* ☐ NO

**If yes, please supply the company name, contact, phone number, and email address.*

RIGGING COMPANY NAME	CONTACT NAME
<input type="text"/>	<input type="text"/>
PHONE NUMBER	EMAIL ADDRESS
<input type="text"/>	<input type="text"/>

3. Is a lift gate needed on the delivery truck? ☐ YES ☐ NO

4. Does the facility have a forklift with a minimum of 5' (152 cm) forks? (Extension forks may be required.)

☐ YES ☐ NO*

**If no, please describe options for removal of the system from the base of the crate.*

5. Will a pallet jack be available? ☐ YES ☐ NO

PATHWAY TO FINAL POSITION

As a reminder, the minimum dimensions to consider when moving the uncrated system (with available touch screen control panel folded in) to the final position are as follows: width of 75.4" (1915 mm), depth of 46.32" (1177 mm), and height of 54.5" (1384 mm).

1. How will the system be transported through the facility (forklift, heavy equipment casters, etc.)?

2. Are steps present in the pathway? ☐ YES* ☐ NO

**If yes, how many steps, are they ascending (up) or descending (down)? Where are they located? What are the dimensions of the stairway (width, depth, and height)?*

IF STEPS ARE PRESENT, A RIGGING COMPANY MAY BE REQUIRED.

3. Will placement require an elevator? ☐ YES* ☐ NO

**If yes, what are the dimensions of the elevator door (height and width) and elevator interior (width, depth, and height)?*

**ELEVATOR WITH LIFT CAPACITY GREATER THAN 1,100 LBS. (500 KG) IS REQUIRED.*

4. Door(s) to pass through? ☐ YES* ☐ NO

**If yes, how many and what are the dimensions (width and height) of each door?*

5. Are there obstacles preventing movement and placement of the system? ☐ YES* ☐ NO

**If yes, what are they, and what is proposed to bypass them?*

6. Is it required for the laser system to be detached from its carts for movement to the installation location?

☐ YES* ☐ NO

**A RIGGING COMPANY AND A ULS SERVICE TECHNICIAN MAY BE REQUIRED.*

PART D - Customer Site Survey & Readiness Requirements Acknowledgement

CUSTOMER ACKNOWLEDGEMENT

I acknowledge that I understand the requirements and that the facility meets all requirements or will meet all requirements for system installation by the latest date listed above.

PRINTED NAME

TITLE

SIGNATURE

DATE